

AQF MR 026E Materials

Determination of chlorine in pigment _____ 1/2

Instruments : AQF-2100H System, HF-210, GA-210, ABC-210/ASC240S

Method : Combustion-ion chromatography

Related standard :

It is critically important to know the chlorine content in the sample for quality control. Concentrations of fluorine, chlorine, bromine, iodine, and sulfur can be determined and accurately by using a combustion ion chromatography (CIC) system combining an Automatic Quick Furnace Model AQF-2100H which safely combusts samples with an ion chromatograph.

Sample name	Pigment
Sample status	
Measuring items	Chlorine (Cl)
Measurement principle	<p>Sample is thermally decomposed in argon (Ar) atmosphere, then combusted in oxygen (O_2) atmosphere. Halogens in the sample are converted to hydrogen halide and halogen gas and sulfur turns into sulfur oxide. These components are collected into absorbing solution and converted to halide ion and sulfate ion. The resulting solution is analyzed by injecting into an ion chromatograph (IC).</p> <p>Analyzing flow [Sample weighing]→[Combustion]→[Collection of combustion gas]→[IC analysis]</p>
Parameters	<p>1. AQF-2100H</p> <div style="margin-left: 40px;"> Sample size : 80mg Sample boat : Ceramic sample boat, SXSMBS Additive : WO_3 100mg Pyrolysis tube : Quartz tube filled with quartz wool Absorbent : Hydrogen peroxide / water </div> <div style="margin-top: 20px;"> HF-210 Heater Temp. Inlet : 1000degC Outlet : 1100degC Gas flow Ar : 200 ml/min O_2 : 400 ml/min </div> <div style="margin-top: 20px;"> GA-210 Absorbent volume : 5ml Sampling loop : 100 ul Absorption tube : For 10 ml Water supply : 2 Ar flow for water supply : 100 ml/min </div>

Sheet No.

AQF MR 026E Determination of chlorine in pigment


2/2

2. Ion chromatograph

Ion chromatograph : DIONEX ICS-1500
 Column : DIONEX Ion Pack AG12A / Ion Pack AS12A
 Eluent : 2.7mM Na₂CO₃ / 0.3mM NaHCO₃
 Eluent flow : 1.50ml / min
 Detector : Conductivity
 Suppressor : ASRS-4-mm
 Measuring time : 30min
 Sampling loop : 100 µl using GA-210 sampling loop
 Calibration : F Cl Br S :0.1ppm ~ 10ppm

Results

Chromatogram

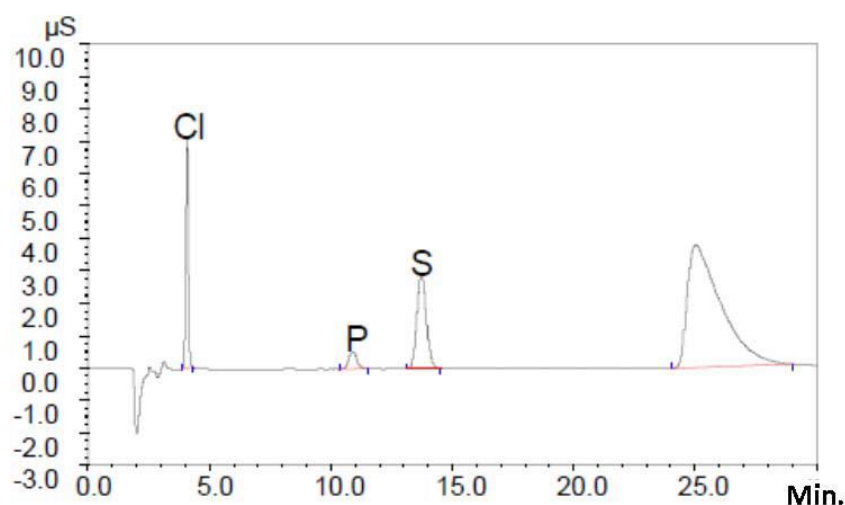

Results

	Cl	1st	2nd	3rd	Average(ppm)	RSD(%)
Pigment 1		222	226	234	227	2.6
Pigment 2		62.7	64.0	65.3	64.0	2.0

Remarks

*Handling of reagents: Confirm labels and safety data sheets of reagents and handle them with enough care.
 *Automation is possible by using an Automatic Sample Changer, ASC-240S.
 When ASC-240S is used, the boat to be used will be a ceramic boat, TX3SCX.

*This application sheet is provided as reference, and does not assure the measurement results. Please consider analysis environment, external factors and sample nature for optimal conditions before the measurement.

AQF2100H_11_010E